

ULTRASOUND AND COMPUTED TOMOGRAPHY  
CARDIAC IMAGE REGISTRATION

CHIENG THION MING

A thesis submitted in fulfillment of the  
requirements for the award of the degree of  
Master of Philosophy (Biomedical Engineering)

Faculty of Biosciences and Medical Engineering  
Universiti Teknologi Malaysia

FEB 2017

Specially dedicated to my beloved family

## ACKNOWLEDGEMENT

All thanks to God for His encouragements and blessings throughout my research where I managed to give my best to accomplish this research.

First and foremost, I would like to express my deepest gratitude to my hardworking supervisor, Dr. Zaid Omar for his words of encouragement, immense support, supervision and financial aid for the entire duration of my study which allows me to breakthrough from challenges to challenges. I would also like to express my gratitude to my co-supervisor, Dr. Nasrul Humaimi Mahmood for his suggestions and recommendations during this research study.

I would like to convey my appreciation to the Ministry of Higher Education (MOHE), Research Management Centre (RMC) and Universiti Teknologi Malaysia (UTM) for supporting my tuition fees, research expenses and living costs through MYBrain15 (MYMASTER) and Flagship grants (Vot 01G16, 01G61 and 12H72). In addition, I wish to thank my research centre, IJN-UTM cardiovascular engineering centre, National Heart Institute of Malaysia (Institut Jantung Negara, IJN) and their medical staffs, especially Dr. Suhaini Kadiman, En. Zaidi, En. Wan Azhar and En. Rizal for their assistance and guidance during my short internship at IJN.

Last but not least, I am grateful to my beloved family members for their unfailing love, trust and patience.

## ABSTRACT

As the trend of the medical intervention moves towards becoming minimally invasive, the role of medical imaging has grown increasingly important. Medical images acquired from a variety of imaging modalities require image preprocessing, information extraction and data analysis algorithms in order for the potentially useful information to be delivered to clinicians so as to facilitate better diagnosis, treatment planning and surgical intervention. This thesis investigates the employment of an affine registration method to register the pre-operative Computed Tomography (CT) and intra-operative Ultrasound cardiac images. The main benefit of registering Ultrasound and CT cardiac images is to compensate the weaknesses and combine the advantages from both modalities. However, the multimodal registration is a complex and challenging task since there is no specific relationship between the intensity values of the corresponding pixels. Image preprocessing methods such as image denoising, edge detection and contour delineation are implemented to obtain the salient and significant features before the registration process. The features-based Scale Invariant Feature Transform (SIFT) method and homography transformation are then applied to find the transformation that aligns the floating image to the reference image. The registration results of three different patient datasets are assessed by the objective performance measures to ensure that the clinically meaningful result are obtained. Furthermore, the relationship between the pre-operative CT image and the transformed intra-operative Ultrasound image are evaluated using joint histogram, MI and NMI. Although the proposed framework falls slightly short of achieving the perfect compensation of cardiac movements and deformation, it can be legitimately implemented as an initialisation step for further studies in dynamic and deformable cardiac registration.

## ABSTRAK

Dengan perubahan trend campur tangan perubatan yang semakin ke arah minimal, peranan pengimejan perubatan telah menjadi semakin penting. Imej-imej perubatan yang diperoleh daripada pelbagai kaedah pengimejan memerlukan pra pemprosesan, pengekstrakan maklumat dan algoritma analisa data bagi maklumat yang berguna agari dihantar kepada doktor untuk memudahkan diagnosis yang lebih baik, perancangan rawatan dan pembedahan. Tesis ini mengkaji pendekatan bagi kaedah pendaftaran secara affine untuk mendaftarkan Computed Tomography (CT) yang bersifat pra-pembedahan dan Ultrasound imej jantung yang bersifat sewaktu-pembedahan. Manfaat utama mendaftarkan imej Ultrasound dan CT jantung adalah untuk mengimbangi kelemahan dan menggabungkan kelebihan daripada kedua-dua kaedah. Walaubagaimanapun, pendaftaran pelbagai pengimejan adalah satu tugas yang kompleks dan mencabar kerana tidak ada hubungan tertentu antara nilai keamatan piksel sepadan. Kaedah pemprosesan imej seperti nyah-hingar, pengesanan titik hujung dan persempadanan kontur dilaksanakan untuk mendapatkan ciri-ciri utama dan penting sebelum proses pendaftaran. SIFT dan transformasi homografi kemudiannya digunakan untuk mencari transformasi yang menjajarkan imej terapung dengan imej rujukan. Keputusan pendaftaran tiga set data pesakit yang berbeza dinilai dengan ukuran objektif untuk memastikan keputusan klinikal yang sesuai diperolehi. Tambahan pula, hubungan antara imej pra-pembedahan CT dan imej sewaktu-pembedahan Ultrasound yang berubah dinilai menggunakan histogram bersama, MI dan NMI. Walaupun rangka kerja yang dicadangkan tidak mencukupi untuk mencapai pampasan yang sempurna pergerakan jantung dan ubah bentuk, ia boleh secara sah dilaksanakan sebagai langkah pengawalan untuk melanjutkan pelajaran dinamik dan pendaftaran jantung ubah bentuk.

## TABLE OF CONTENTS

CHAPTER	TITLE	PAGE
	<b>DECLARATION</b>	ii
	<b>DEDICATION</b>	iii
	<b>ACKNOWLEDGEMENT</b>	iv
	<b>ABSTRACT</b>	v
	<b>ABSTRAK</b>	vi
	<b>TABLE OF CONTENTS</b>	vii
	<b>LIST OF TABLES</b>	x
	<b>LIST OF FIGURES</b>	xi
	<b>LIST OF SYMBOLS</b>	xv
	<b>LIST OF ABBREVIATIONS</b>	xvi
	<b>LIST OF APPENDICES</b>	xviii
<b>1</b>	<b>INTRODUCTION</b>	1
	1.1 Introduction	1
	1.2 Research Background	2
	1.3 Problem Statement	3
	1.4 Research Objectives	5
	1.5 Research Scopes	6
	1.6 Structure of Thesis	7
<b>2</b>	<b>LITERATURE REVIEW</b>	8
	2.1 Introduction	8

2.2	The Heart	9
2.2.1	The Anatomical Structure of Heart	9
2.2.2	The Characteristics of Heart	11
2.3	The Basic Physics of Cardiac Imaging Modalities	12
2.3.1	Ultrasound Imaging	12
2.3.2	Computed Tomography Imaging	15
2.3.3	Correlating Issues between Ultrasound and CT images	18
2.4	Medical Image Registration	19
2.5	Classification of Registration Method	21
2.5.1	Extrinsic Registration	21
2.5.2	Intrinsic Registration	23
2.5.2.1	Anatomical Landmarks-based Methods	23
2.5.2.2	Segmentation-based Methods	24
2.5.2.3	Intensity-based Methods	25
2.5.2.4	Hybrid Methods	28
2.6	Domain and Nature of the Transformation	32
2.7	Optimization Process	34
2.9	Medical Image Fusion	35
2.8	Summary	36
<b>3</b>	<b>RESEARCH METHODOLOGY</b>	<b>37</b>
3.1	Introduction	37
3.2	Preprocessing Stage	39
3.2.1	Ultrasound Preprocessing Steps	39
3.2.2	CT Preprocessing Steps	43
3.3	Feature Extraction Stage	49
3.4	Registration Stage	54
3.5	Similarity Measure Stage	62
3.6	Summary	65

<b>4</b>	<b>EXPERIMENTAL RESULTS AND DISCUSSIONS</b>	<b>66</b>
4.1	Introduction	66
4.2	Cardiac Image Acquisition	66
4.3	Preprocessing Stage	68
4.3.1	Ultrasound Preprocessing Steps	68
4.3.2	CT Preprocessing Steps	72
4.4	Feature Extraction Stage	78
4.5	Registration Stage	82
4.6	Similarity Measure Stage	90
4.7	Summary	95
<b>5</b>	<b>CONCLUSIONS AND FUTURE WORKS</b>	<b>96</b>
5.1	Conclusion	96
5.2	Suggestion for Future Works	98
	<b>REFERENCES</b>	<b>100</b>
	Appendices A-F	114-145



## LIST OF TABLES

TABLE NO.	TITLE	PAGE
2.1	CT number (HU) with respective substances	16
2.2	Comparison between different image registration approaches	30
4.1	Patient label and their respective MRN number	68
4.2	Performance evaluation and comparison using the image quality metrics for the experimental results obtained with the datasets of Patient A	77
4.3	Computational time of the GVF snake technique in delineating the closed contours of the targeted feature for Patient A datasets	81
4.4	Statistical analysis of the SIFT registration results obtained with the Patient A datasets	87
4.5	Performance evaluation using histogram comparison methods with the Patient A datasets	88
4.6	Intensity-based similarity measure criteria computed with the transformed Ultrasound dataset and its corresponding CT cardiac image of Patient A.	92
4.7	Intensity-based similarity measure criteria computed with the pre- registered Ultrasound dataset and its corresponding CT cardiac image of Patient A.	92
4.8	Similarity measurement of the mutual information and normalized mutual information values that obtained with the transformed datasets and pre-registered datasets of Patient A.	93
4.9	Intensity-based similarity measure criteria computed with the registration results obtained from the intensity-based method and its corresponding CT cardiac image of Patient A.	93

## LIST OF FIGURES

<b>FIGURE NO.</b>	<b>TITLE</b>	<b>PAGE</b>
1.1	Overview and workflow of the real-time Ultrasound and CT cardiac image-guided intervention system proposed by IJN-UTM Cardiovascular Engineering Centre	6
2.1	The anterior view of human heart	10
2.2	Reflection, refraction, absorption and scattering process of ultrasound echoes	14
2.3	Block diagram of a common image registration framework	20
2.4	The domain and nature of the transformation	33
3.1	The workflow of the proposed framework	38
3.2	Block diagram of the proposed methodology	38
3.3	Block diagram of the Ultrasound preprocessing steps	39
3.4	Block diagram of the CT preprocessing steps	43
3.5	Six different structuring elements used in the morphological based edge detection method	44
3.6	(a) Convergence of the traditional snake technique with (b) traditional potential forces, and (c) shown the close-up within the boundary concavity.	51
3.7	(a) Convergence of the GVF snake technique with (b) GVF potential forces, and (c) shown the close-up within the boundary concavity.	53
3.8	Block diagram of the image registration stage	54

3.9	General workflow of the Scale Invariant Feature Transform (SIFT) algorithm	54
3.10	Scale-space extreme detection	56
3.11	Key-point descriptor with total 128 element feature vectors	58
3.12	Joint histogram of the reference image, $A$ and transformed image, $B$	64
3.13	Joint histogram of two completely similar images	64
4.1	Siemens Syngo Multimodality Workplace (MWP)	67
4.2	(a) Ultrasound cardiac image of the Patient A with apical two chamber view. (b) Speckle-free Ultrasound image, after smoothing using SRAD technique. (c) Denoised and enhanced Ultrasound image. (d) Optimal Ultrasound edges extracted by the proposed framework. (e) Ultrasound cardiac image with the highlighted edges.	70
4.3	(a) Ultrasound cardiac image of the Patient A with apical four chamber view, (d) parasternal long axis view and (g) parasternal short axis view. (b), (e), and (h) are their respective denoised images obtained with the proposed framework. (c), (f), and (i) are the respective optimal edges extracted by the proposed framework	71
4.4	(a) CT cardiac image of the Patient A with apical two chamber view. (b) Artifacts and unwanted noises computed from median filter and basic morphology filter. (c) Denoised and enhanced CT image. (d) Optimal CT edges extracted by the proposed framework. (e) CT cardiac image with the highlighted edges.	73
4.5	(a) CT cardiac image of the Patient A with apical four chamber view, (d) parasternal long axis view and (g) parasternal short axis view. (b), (e) and (h) are their respective denoised images obtained with the proposed framework. (c), (f) and (i) are their respective CT cardiac image with the edges that extracted by the proposed framework (highlighted in green colour).	74

- 4.6 (a) Edges extracted from the Patient A CT dataset with apical two chamber view using the Canny operator, (b) Sobel operator, (c) Kumar's method and (d) proposed method. (e) Edges extracted from the Patient A CT dataset with apical four chamber view using the Canny operator, (f) Sobel operator, (g) Kumar's method and (h) proposed method. (i) Edges extracted from the Patient A CT dataset with parasternal long axis view using the Canny operator, (j) Sobel operator, (k) Kumar's method and (l) proposed method. (m) Edges extracted from the Patient A CT dataset with parasternal short axis view using the Canny operator, (n) Sobel operator, (o) Kumar's method and (p) proposed method. 75
- 4.7 (a) Ultrasound cardiac image of the Patient A with apical two chamber view, (d) apical four chamber view, (g) parasternal long axis view and (j) parasternal short axis view. (b), (e), (h) and (k) are their respective initial contour selected manually by the operator (red contour). (c), (f), (i) and (l) are their respective closed contour delineated by the GVF snake technique (blue contour). 78
- 4.8 (a) CT cardiac image of the Patient A with apical two chamber view, (d) apical four chamber view, (g) parasternal long axis view and (j) parasternal short axis view. (b), (e), (h) and (k) are their respective initial contour selected manually by the operator (red contour). (c), (f), (i) and (l) are their respective closed contour delineated by the GVF snake technique (blue contour). 79
- 4.9 (a) Ultrasound cardiac images of the Patient A with apical two chamber view and (b) its corresponding CT image, where the blue contours are the closed contour delineation by the GVF snake technique in the previous stage. 83
- 4.10 Good matching between the Ultrasound image (floating image, on the left-hand side) and pre-registered Ultrasound image (reference image, on the right-hand side) of the Patient A dataset with apical two chamber view 84
- 4.11 (a) CT cardiac image of the Patient A with apical two chamber view. (b) The corresponding Ultrasound image is transformed based on the computed homography matrix,  $H$ . (c) Overlapping image of the transformed Ultrasound image and corresponding CT cardiac image. 84

- 4.12 Good matching between the Ultrasound image (floating image, on the left-hand side) and pre-registered Ultrasound image (reference image, on the right-hand side) of the Patient A dataset with (a) apical four chamber view, (b) parasternal long axis view and (c) parasternal short axis view 85
- 4.13 CT cardiac image of the Patient A with (a) apical four chamber view, (d) parasternal long axis view and (g) parasternal short axis view. (b), (e) and (h) are their corresponding transformed Ultrasound images based on the computed homography matrix,  $H$ . (c), (f) and (i) are their respective overlapping images of the transformed Ultrasound and CT cardiac images. 86
- 4.14 CT cardiac image of the Patient A with (a) apical two chamber view, (d) apical four chamber view, (g) parasternal long axis view and (j) parasternal short axis view. (b), (e), (h) and (k) are their corresponding transformed Ultrasound images using the intensity-based registration method. (c), (f), (i) and (l) are their respective overlapping images of the transformed Ultrasound and CT cardiac images. 89
- 4.15 Joint histogram constructed using the transformed datasets of Patient A with (a) apical two chamber view, (b) apical four chamber view, (c) parasternal long axis view and (d) parasternal short axis view 91

**LIST OF SYMBOLS**

$\theta$	-	Angle
$*$	-	Convolution Operator
$\oplus$	-	Dilation Operator
$\ominus$	-	Erosion Operator
$\circ$	-	Opening Operator
$\bullet$	-	Closing Operator
$\infty$	-	Infinity
$\mu$	-	Attenuation Coefficient
$\sigma$	-	Standard Deviation

**LIST OF ABBREVIATIONS**

2D	-	2 Dimensional
3D	-	3 Dimensional
4D	-	4 Dimensional
CAT	-	Computerized Axial Tomography
CC	-	Correlation Coefficient
CDF	-	Cumulative Distribution Function
CLAHE	-	Contrast Limited Adaptive Histogram Equalization
CT	-	Computed Tomography
CVDs	-	Cardiovascular diseases
DICOM	-	Digital Imaging and Communications in Medicine
DLT	-	Direct Linear Transform
DOF	-	Degree of Freedom
DoG	-	Difference of Gaussian
ECG	-	Electrocardiogram
GVF	-	Gradient Vector Flow
HU	-	Hounsfield Units
ICP	-	Iterative Closest Point
MAE	-	Mean Absolute Error
MI	-	Mutual Information
MRI	-	Magnetic Resonance Imaging
MRN	-	Patient's Medical Record
MSE	-	Mean Square Error
MWP	-	Multimodality Workplace
NCC	-	Normalized Cross Correlation
NMI	-	Normalized Mutual Information

PDE	-	Partial Differential Equation
PET	-	Positron Emission Tomography
PSNR	-	Peak Signal to Noise Ratio
RANSAC	-	RANdom SAmples Consensus
SAD	-	Sum of Absolute Differences
SIFT	-	Scale Invariant Feature Transform
SPECT	-	Single-Photon Emission Computerized Tomography
SRAD	-	Speckle Reducing Anisotropic Diffusion
SSD	-	Sum of Squared Differences
SSIM	-	Structural Similarity Index Metric
TEE	-	Transesophageal Echocardiography
TRE	-	Target Registration Error
VFC	-	Vector Field Convolution



**LIST OF APPENDICES**

<b>APPENDIX</b>	<b>TITLE</b>	<b>PAGE</b>
A	Ultrasound Preprocessing Stage	114
B	CT Preprocessing Stage	117
C	Feature Extraction Stage	125
D	Registration Stage	132
E	Similarity Measure Stage	139
F	List of Publication	145

## **CHAPTER 1**

### **INTRODUCTION**

#### **1.1 Introduction**

Cardiovascular diseases (CVDs) are diseases of the heart and blood vessel, including coronary heart disease, cerebrovascular disease, peripheral arterial disease, rheumatic heart disease and congenital heart disease [1]. They are also known as heart and circulatory disease. The most common cause of CVDs is atherosclerosis, which is the build-up of plaques on the inner walls of the arteries that limits or blocks the blood supply to the heart or brain. This can lead to serious health problems such as heart attack, heart failure, stroke or even death. According to the report “Heart disease and stroke statistic–2015 update” published by American Heart Association [1], CVDs remain the leading global cause of death with 17.3 million deaths each year. The number is expected to exceed 23.6 million by 2030, and 80% of CVD deaths occurred in low-income and middle-income countries [1]. The estimated global cost of direct and indirect loss, including healthcare expenditure and loss of productivity was 863 billion in 2010 and is expected to rise to \$1.04 trillion in 2030 [2]. Therefore, it is essential to have effective and low cost healthcare services available for the general population, thus able to contribute to more saving of lives.

## 1.2 Research Background

Medical imaging is experiencing a significant growth and becoming an integral part in modern healthcare, due to the rapid development of computing power and the improvements in imaging technologies over the past few decades. Medical imaging has been extensively used for the purpose of diagnosis, disease monitoring, treatment planning, and surgical intervention. There are several medical imaging devices that are widely available, such as Computed Tomography (CT), Magnetic Resonance Imaging (MRI), Positron Emission Tomography (PET), Ultrasound, Single-Photon Emission Computerized Tomography (SPECT), X-ray, and more. The images acquired from these devices display the anatomical structure and functional information about a human organ. They are usually raw in nature and require subsequent preprocessing, information extraction and data analysis in order for the potentially useful information to be benefitted. In this regard, quantitative evaluation and assessment of medical images, using computer-aided imaging techniques, has enabled the clinicians in reaching an unbiased and more objective decision within a short span of time [3, 4].

Furthermore, the role of medical imaging has expanded beyond the visualization of anatomical structure and functional information of the organ, as it continues to develop into advanced clinical tools such as image-guided intervention [5, 6]. Image-guided intervention is the procedure that uses sophisticated imaging technology and computer-assisted systems to provide the information required by the clinicians to visualize and locate the surgical areas precisely [6]. It has become an essential medical procedure for cardiovascular diseases due to its minimally invasive characteristics, which is capable of performing the intervention by inserting catheters into the heart rather than opening up the heart. The advantages of minimally invasive intervention are numerous, including smaller incisions, lower risk of bleeding, lower risk of infection and shorter recovery time compared to open surgery [7].

However, minimally invasive intervention is not without its limitations; notably it has less or no direct open visual inspection with the surgical target and tool. Hence, the process of extracting, registering and combining the information acquired from medical images are required in providing a detailed road map that can lead to a successful image guided intervention [6]. It is known that different medical imaging modalities brings different complementary and advantageous information for different clinical applications. Each modality has different clinical domains and a range of applicability [8]. For example, CT acquires images of anatomical structures of the organ with high spatial resolution and high contrast between bones and tissues. MRI meanwhile, is mainly used for the imaging of soft tissues. PET and SPECT provide functional and metabolic information which allows the detection of a tumor and highlight its activities. On the other hand, Ultrasound imaging offers a non-invasive solution and real-time capability in guiding intervention. Based on all the above, it is clearly not possible for a single imaging modality aforementioned to comprehensively derive all details required to facilitate a proper diagnosis, treatment planning and intervention. Therefore, image fusion technique is used as solution to combine all information under one modality. A pre-requisite of fusion is a procedure known as image registration.

### **1.3 Problem Statement**

Image registration technique is used to establish the correspondence or spatial mapping between sets of image data. It has a wide variety of applications in the field of remote sensing, computer vision, robotics and medical image processing. In medical imaging, the registration process aim to discover the transformation that spatially and geometrically aligns two or more images that are acquired from the same or different subjects, from the same or different modalities, at the same or different viewpoint and at a same or different time [9, 10]. It enables the establishment of the correspondence between the target image and the reference image by mapping the correlated point or feature in one coordinate space into

another coordinate space. The choice of modalities reflects real world situations. The high temporal resolution, non-invasive and real-time intra-operative Ultrasound image is registered with high spatial resolution pre-operative CT image in order to explore the possibility of implementing the real-time Ultrasound and CT cardiac image guided intervention system.

Nevertheless, multi-modal image registration is a unique, complex and challenging task in the medical imaging field. The reasons for this is described as follows: different imaging modalities use different principles and parameters in their acquisition process. Hence, different imaging modality devices tend to produce the images with different characteristics and different physical representations, even for the same target organ [11]. In other words, the correlation between the images of different imaging modalities are relatively low. Thus, the contrast in image properties, viewing size, angle and position between the respective imaging modalities may become the obstacles.


Another issue is a forced compromise between spatial resolution and temporal resolution of an image. The medical image with high spatial resolution usually does not have good temporal resolution and vice versa. Registration of Ultrasound and CT images ensures compensation of the spatial and temporal difference, and the information acquired from both modalities can be integrated [12,13]. This in turn can greatly assist the clinician in locating targeted regions and making objective decisions during the intervention. Besides that, due to no specific or unknown relationship between the intensity values of the corresponding pixels of intra-operative Ultrasound image and pre-operative CT image acquired from the patient in the operating room, registration becomes much more difficult process [14]. In addition, there is still no standard procedure or fully automated registration method available to handle various clinical applications. Thus, multimodal cardiac image registration remains as an open and challenging research area.

## 1.4 Research Objectives

The research proposed in this thesis is part of a larger research framework that aims to implement real-time Ultrasound and Computed Tomography cardiac image-guided intervention system. It has been the central aim of collaborative research efforts at the IJN-UTM Cardiovascular Engineering Centre, Universiti Teknologi Malaysia. The overview and workflow of the proposed system are shown in Figure 1.1. The red-dotted box is the main focus of this thesis.

Based on the problem statement, the objectives of this research are stated as follows:

- i. To preprocess and extract the salient features from the intra-operative Ultrasound cardiac image and pre-operative CT cardiac image, respectively.
- ii. To register the intra-operative Ultrasound cardiac image and pre-operative CT cardiac image via a feature-based registration method.
- iii. To assess and evaluate the performance of the proposed Ultrasound-CT image registration framework using an intensity-based similarity measure.

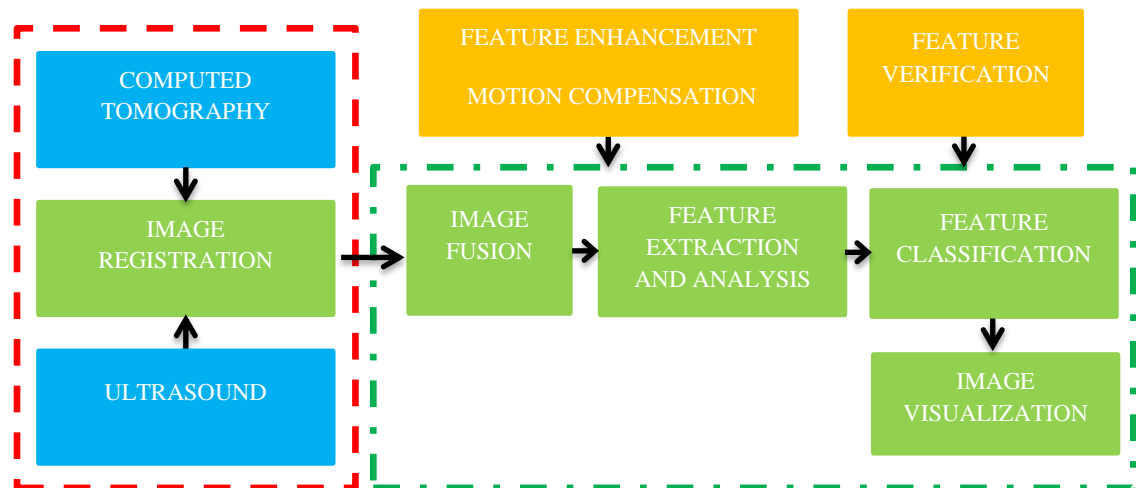

**Figure 1.1:** Overview and workflow of the real-time Ultrasound and CT cardiac image-guided intervention system proposed by IJN-UTM Cardiovascular Engineering Centre

## 1.5 Research Scopes

Several scopes have been outlined for this research:

- i. Two-dimensional (2D) Ultrasound and CT cardiac images are used.
- ii. Three randomly selected patient datasets are acquired from IJN and used throughout this research.
- iii. Includes only four different basic Ultrasound cardiac views: apical two chamber view, apical four chamber view, parasternal long axis view and parasternal short axis view at the papillary muscle level. A total of 24 images are therefore used in this thesis.

- iv. Affine transformation which is invariant to translation, rotation, shearing and scaling, are considered.
- v. Pre-registered or manually registered Ultrasound datasets constructed by the IJN medical practitioner, are used as the reference image in determining the geometrical transformation that maps and aligns the Ultrasound and CT cardiac images.

## **1.6 Structure of Thesis**

This thesis consists of five chapters and is organized as follows: Chapter One presents the introduction of the research study. This chapter includes an introduction, research background, problem statements, research objectives, research scope and structure of the thesis. Chapter Two describes the anatomical structure of the heart. The basic physic of the Ultrasound and CT imaging modalities also discussed in this chapter. Next, the literature review related to the medical image registration methods is studied, thus pointing out their strengths and limitations respectively. Chapter Three highlights the detail of the proposed methodology and techniques used for the registration framework. It consists of four main stages: preprocessing stage, feature extraction stage, registration stage and similarity measure stage. Chapter Four presents and discusses the experimental findings obtained using patient datasets for each stage. Lastly, Chapter Five summarizes and concludes the thesis along with the recommendations for future work.





## REFERENCE

- [1] Mozaffarian, D., Benjamin, E. J., Go A. S., Arnett, D. K., Blaha M. J., Cushman, M. Heart Disease and Stroke Statistics--2015 Update: *American Heart Association Circulation*, 2015. 131(4):e29-322.
- [2] Bloom, D. E., Cafiero, E. T., Jané-Llopis, E., Abrahams-Gessel, S., Bloom, L. R., Fathima, S., Feigl, A. B., Gaziano, T., Mowafi, M., Pandya, A., Prettner, K., Rosenberg, L., Seligman, B., Stein, A. Z., and Weinstein, C. *The Global Economic Burden of Noncommunicable Diseases*. Geneva, Switzerland: Harvard School of Public Health, World Economic Forum; 2011.
- [3] James, A. P., and Dasarathy, B. V. Medical Image Fusion: A Survey of the State of the Art. *Information Fusion*. 2014. 19:4-19.
- [4] Russell, T., and Joskowicz, L. Computer-Integrated Surgery and Medical Robotics. In: M Kutz. *Standard Handbook of Biomedical Engineering*. 325-53; 2002.
- [5] McInerney, T., and Terzopoulos, D. Deformable Models in Medical Image Analysis: A Survey. *Medical Imaging Analysis*. 1996. 1(2): 91-108.
- [6] Cleary, K., and Peters, T. M. Image-guided Interventions: Technology Review and Clinical Applications. *Annual review of biomedical engineering*. 2010. 12:119-42.
- [7] Iribarne, A., Easterwood, R., Chan, E. Y., Yang, J., Soni, L., Russo, M. J., et al. The Golden Age of Minimally Invasive Cardiothoracic Surgery: Current and Future Perspectives. *Future Cardiol*. 2011. 7(3):333-46.
- [8] Demongeot, J., Wendling, J. B., Mattes, J., Haigron, P., Glade, N., and Coatrieux, J. L. Multiscale Modeling and Imaging: The Challenges of Biocomplexity. *Proceedings of the IEEE*. 2003. 91(10):1723-37.

- [9] Oliveira, F. P. M. and Tavares, J. M. R. Medical Image Registration: A Review. *Computer Methods in Biomechanics and Biomedical Engineering*. 2014. 17(2): 73-93
- [10] Xiong, Z. and Zhang, Y. A Critical Review of Image Registration Methods. *International Journal of Image and Data Fusion*. 2010.1(2): 137-58.
- [11] Curiel, L., Chopra, R. and Hynynen, K. Progress in Multimodality Imaging: Truly Simultaneous Ultrasound and Magnetic Resonance Imaging. *IEEE transactions on medical imaging*. 2007. 26(12):1740-6.
- [12] Wein, W., Brunke, S., Khamene, A., Callstrom, M. R., Navab, N. Automatic CT-Ultrasound Registration for Diagnostic Imaging and Image-guided Intervention. *Medical Image Analysis*. 2008. 12(5): 577-585.
- [13] Lang, P., Rajchl, M., Li, F. and Peters, T. M. Towards Model-enhanced Real-time Ultrasound Guided Cardiac Interventions. *IEEE International Conference on Intelligent Computation and Bio-Medical Instrumentation (ICBMI)*, December, 2011. 89-92.
- [14] Rogelj, P., S. Kovačič, and Gee, J.C. Point similarity measures for non-rigid registration of multi-modal data. *Computer Vision and Image Understanding*, 2003. 92(1): 112-140.
- [15] Tortora, G. J. and Derrickson, B. H. *Principles of Anatomy and Physiology: Maintenance and Continuity of the Human Body*. Volume 2: John Wiley & Sons, Incorporated. 2008;717-59.
- [16] Tavakoli, V. and Amini, A. A. A Survey of Shaped-based Registration and Segmentation Techniques for Cardiac Images. *Computer Vision and Image Understanding*. 2013. 117(9): 966-989.
- [17] Makela, T., Clarysse, P., Sipila, O., Pauna, N., Pham, Q. C., Katila, T. et al. A Review of Cardiac Image Registration Methods. *IEEE Trans Med Imaging*. 2002. 21(9): 1011- 21.
- [18] Shechter, G., Ozturk, C., Resar, J. R. and Mcveigh, E. R. Respiratory Motion of the Heart from Free Breathing Coronary Angiograms. *IEEE Transactions on Medical Imaging*. 2004. 23(8):1046–1056.
- [19] Manke, D., Nehrke, K., Röscher, P. and Dössel, O. Study of Respiratory Motion of the Heart in coronary Angiography. *International Journal of Bioelectromagnetism*. 2000. 2(2).

- [20] Ter-Pogossian, M. M., Bergmann, S. R. and Sobel, B. E. Influence of Cardiac and Respiratory Motion on Tomographic Reconstructions of the Heart: Implications for Quantitative Nuclear Cardiology. *J Comput Assist Tomogr.* 1982. 6(6):1148–1155.
- [21] Klein, G. J. and Huesman, R. H. Four-dimensional Processing of Deformable Cardiac PET Data. *Med Image Anal.* 2002. 6(1): 29-46.
- [22] Fenster, A., Downey, D. B. and Neale Cardinal, H. Three-dimensional Ultrasound Imaging. *Physics in Medicine and Biology.* 2001. 46(5):67-99.
- [23] Burns, P. N. Introduction to the physical principles of Ultrasound imaging and doppler. *Fundamentals in Medical Biophysics.*2005.
- [24] Michailovich, O. V. and Tannenbaum, A. Despeckling of Medical Ultrasound Images. *IEEE Transactions on Ultrasound Ferroelectrics Frequency Control.* 2006. 53(1): 64-78.
- [25] Physical principles of Ultrasound
- [26] Kossoff, G. Basic Physics and Imaging Characteristics of Ultrasound. *World Journal of Surgery.* 2000. 24(2): 134-142.
- [27] Smith, S. W. *The Scientist and Engineer's Guide to Digital Signal Processing.* San Diego: California Technical Publishing. 1997. 442-450.
- [28] Sheikh, N. *Medium Resolution Computed Tomography through Phosphor Screen Detector and 3D Image Analysis.* Doctoral Dissertation. Iowa State University; 2006.
- [29] Ulzheimer, S. and Flohr, T. Multislice CT: Current Technology and Future Developments. In: Reiser, M. F., Becker, C. R., Nikolaou, K. and Glazer, G. ed. *Multislice CT.* Heidelberg: Springer-Berlin. 3-23; 2009.
- [30] Barrett, J. F. and Nicholas, K . Artifacts in CT: Recognition and Avoidance. *RadioGraphics.* 2004. 24(6):1679 – 1691.
- [31] Herrmann, T. L., Fauber, T. L., Gill, J., Hoffman, C., Orth, D. K., Peterson, P. A., Prouty, R. R., Woodward, A. P. and Odle, T. G. Best Practices in Digital Radiography. *Radiologic Technology.* 2012. 84(1): 83-89.
- [32] Herbert, L. F. Drawbacks and Limitations of Computed Tomography. *Texas Heart Institute Journal.* 2004. 31(4): 345-348
- [33] Ratib, O. and Rosset, A. Open-source Software in Medical Imaging: Development of OsiriX. *Int. J. Comput. Assist. Radiol. Surg.* 2006. 1(4): 187–196.

- [34] Brown, L. G. A Survey of Image Registration Techniques. *ACM Comput. Surv.* 1992. 24(4): 325-376.
- [35] Maintz, J. B. A., Viergever, M. A. An Overview of Medical Image Registration Methods. In *Symposium of the Belgian hospital physicists association*. 1996.
- [36] Sonka, M. and Fitzpatrick, J. M. *Handbook of medical imaging*. (Volume 2, Medical image processing and analysis) SPIE- The international society for optical engineering. 2000. 375-435
- [37] Peters, T., Davey, B., Munger, P., Comeau, R., Evans, A. and Olivier, A. Three-dimensional Multimodal Image-guidance for Neurosurgery. *IEEE Transactions on Medical Imaging*. 1996. 15(2): 121-128.
- [38] Ellis, R. E., Toksvig-Larsen, S., Marcacci M., Caramella, D. and Fadda, M. A Biocompatible Fiducial Marker for Evaluating the Accuracy of CT Image Registration. In Lemke, H. U., Vannier, M. W., Inamura, K. and Farman, A. G. ed., *Computer assisted radiology, volume 1124 of Excerpta medica-international congress series*. Amsterdam: Elsevier. 693-698; 1996.
- [39] Wang, M. Y., Fitzpatrick, J. M., Maurer, C. R. and Maciunas, R. J. An Automatic Technique for Localizing Externally Attached Markers in MR and CT Volume Images of the Head. In Loew, M. H. ed. *Medical imaging: image processing*. Bellingham, WA: SPIE Press. Vol. 2167: 214–224; 1994.
- [40] Huang, X., Moore, J., Guiraudon, G., Jones, D. L., Bainbridge, D., Ren, J. et al. Dynamic 2D Ultrasound and 3D CT Image Registration of the Beating Heart. *IEEE transactions on medical imaging*. 2009. 28(8):1179-89.
- [41] Mani, V. R. S. and Rivazhagan, D. S. Survey of Medical Image Registration. *Journal of Biomedical Engineering and Technology*. 2013. 1(2):8-25.
- [42] Faber, T. L., McColl, R. W., Opperman, R. M., Corbett, J. R. and Peshock, R. M. Spatial and Temporal Registration of Cardiac SPECT and MR Images: Methods and Evaluation. *Radiology*. 1991. 179(3): 857-861.
- [43] Pallotta, S., Gilardi, M.C., Bettinardi, V., Rizzo, G., Landoni, C., Striano, G., Masi, R. and Fazio, F. Application of a Surface Matching Image Registration Technique to the Correlation of Cardiac Studies in Positron Emission Tomography (PET) by Transmission Images. *Physics in medicine and biology*. 1995. 40(10): 1695-1708.

- [44] Fright, W.R. and Linney, A.D. Registration of 3-D Head Surfaces using Multiple Landmarks. *IEEE Transactions on Medical Imaging*. 1993. 12(3): 515-520.
- [45] Gilardi, M. C., Rizzo, G., Savi, A. and Fazio, F. Registration of multimodal biomedical images of the heart. *Q. J. Nucl. Med.* 1996. 40(1): 142-150.
- [46] McParland, B. J. and Kumaradas, J. C. Digital Portal Image Registration by Sequential Anatomical Matchpoint and Image Correlations for Real-time Continuous Field Alignment Verification. *Medical physics*. 1995. 22(7): 1063-1075.
- [47] Savi, A., Gilardi, M. C., Rizzo, G., Pepi, M., Landoni, C., Rossetti, C., Lucignani, G., Bartorelli, A. and Fazio, F. Spatial Registration of Echocardiographic and Positron Emission Tomographic Heart Studies. *European journal of nuclear medicine*. 1995. 22(3): 243-247.
- [48] Sinha, S., Sinha, U., Czernin, J., Porenta, G. and Schelbert, H. R. Noninvasive Assessment of Myocardial Perfusion and Metabolism: Feasibility of Registering Gated MR and PET images. *AJR. American journal of roentgenology*. 1995. 164(2): 301-307.
- [49] Pelizzari, C. A., Chen, G. T., Spelbring, D. R., Weichselbaum, R. R. and Chen, C.T. Accurate Three-dimensional Registration of CT, PET, and/or MR Images of the Brain. *Journal of computer assisted tomography*. 1989. 13(1): 20-26.
- [50] Press, W. H., Teukolsky, S. A., Vetterling, W. T. and Flannery, B. P. *Numerical Recipes in C: The Art of Scientific Computing*, 2<sup>nd</sup> ed. Cambridge, U.K.: Cambridge Univ. Press, 1992
- [51] Borgefors, G. Hierarchical chamfer matching: a parametric edge matching algorithm. *IEEE Transactions on Pattern Analysis and Machine Intelligence*. 1988. 10(6): 849-865.
- [52] M. Van Herk. Image registration using chamfer matching. In *Handbook of Medical Imaging: Processing and Analysis*. NewYork: Academic Press, Inc. 515–527; 2000.
- [53] Declerck, J., Feldmar, J., Betting, F. and Goris, M. L. Automatic registration and alignment on a template of cardiac stress and rest SPECT images. *IEEE Proceedings of the Workshop on Mathematical Methods in Biomedical Image Analysis*. 1996. 212-221.

- [54] H. Zhong, T. Kanade, D. Schwartzman. Virtual Touch: An Efficient Registration Method for Catheter Navigation in Left Atrium. *Medical Image Computing and Computer-Assisted Intervention. MICCAI International Conference on Medical Image Computing and Computer-Assisted Intervention*. 2006. 9(1): 437–44.
- [55] Dandekar, O. High-performance Three-dimensional Image Processing Architectures for Image-guided Interventions. *ProQuest*. 2008.
- [56] Gueziec, A. P. and Ayache, N. Large Deformable Splines, Crest Lines, and Matching. *In SPIE's 1993 International Symposium on Optics, Imaging, and Instrumentation. International Society for Optics and Photonics*. 1993. 316-327.
- [57] McInerney, T. and Terzopoulos, D. Deformable Models in Medical Image Analysis. *IEEE computer society press in Mathematical methods, biomedical image analysis*, Los Alamitos, CA. 1996. 171–180.
- [58] Gaens, T., Maes, F., Vandermeulen, D. and Suetens, P. Non-rigid Multimodal Image Registration using Mutual Information. *In Medical Image Computing and Computer-Assisted Intervention-MICCAI'98*. Heidelberg: Springer Berlin. 1998. 1099-1106.
- [59] Declerck, J., Feldmar, J., Goris, M. L. and Betting, F. Automatic Registration and Alignment on a Template of Cardiac Stress and Rest Reoriented SPECT Images. *IEEE Transactions on Medical Imaging*. 1997. 16(6): 727-737.
- [60] Deriche, R. Using Canny's Criteria to Derive a Recursively Implemented Optimal Edge Detector. *Int. J. Comput. Vision*. 1987. 1(2): 167–187.
- [61] Arata, L. K., Dhawan, A. P., Broderick, J. P., Gaskil-Shipley, M. F., Levy, A.V., Volkow, N. D. Three-dimensional Anatomical Model-based Segmentation of MR Brain Images through Principal Axes Registration. *IEEE transactions on bio-medical engineering*. 1995. 42(11): 1069-78.
- [62] Dong, L. and Boyer, A. L. A Portal Image Alignment and Patient Setup Verification Procedure using Moments and Correlation Techniques. *Physics in medicine and biology*. 1996. 41(4): 697-723.
- [63] Wang, H. and Fallone, B. G. A Robust Morphological Algorithm for Automatic Radiation Field Extraction and Correlation of Portal Images. *Medical physics*. 1994. 21(2): 237-244.

- [64] Pavía, J., Rose, D., Catafau, A. M., Lomeña, F. J., Huguet, M. and Setoain, J., Three-dimensional Realignment of Activation Brain Single-photon Emission Tomographic Studies. *European journal of nuclear medicine*. 1994. 21(12): 1298-1302.
- [65] Roche, A., Malandain, G., Ayache, N. and Prima, S. Towards a Better Comprehension of Similarity Measures used in Medical Image Registration. *Medical Image Computing and Computer-Assisted Intervention–MICCAI'99*. September, 1999. Heidelberg: Springer Berlin. 1999. 555-566.
- [66] Maintz, J. B. A. and Viergever, M. A. A Survey of Medical Image Registration. *Medical Image Analysis*. 1998. 2(1): 1-36.
- [67] Turkington, T. G., DeGrado, T. R., Hanson, M. W. and Coleman, R. E. Alignment of Dynamic Cardiac PET Images for Correction of Motion. *IEEE Transactions on Nuclear Science*. 1997. 44(2): 235-242.
- [68] Bacharach, S. L., Douglas, M. A., Carson, R. E., Kalkowski, P. J., Freedman, N. M., Perrone-Filardi, P. and Bonow, R. O. Three-dimensional Registration of Cardiac Positron Emission Tomography Attenuation Scans. *Journal of nuclear medicine*. 1993. 34(2): 11-321.
- [69] Hajnal, J. V., Hill, D. L. G. and Hawkes, D. J. *Medical Image Registration*. CRC Press: Boca Raton. 2001.
- [70] Fitzpatrick, J. M., Hill, D. L. G. and Maurer, C. R. Image Registration. *Handbook of Medical Imaging (Vol.2)*. Bellingham, WA: SPIE Press. 375–435; 2000.
- [71] Sun, Y., Kadoury, S., Li, Y., John, M., Resnick, J., Plambeck, G., Liao, R., Sauer, F. and Xu, C. Image Guidance of Intracardiac Ultrasound With Fusion of Pre-Operative Images. *Int. Conf. Med. Image Comput. Comput. Assist. Interv.* 2007. 10(1): 60–67.
- [72] Wells, W. M., Viola, P., Atsumi, H., Nakajima, S. and Kikinis, R. Multi-modal Volume Registration by Maximization of Mutual Information. *Medical image analysis*. 1996. 1(1): 35-51.
- [73] Woods, R. P. Within-modality Registration using Intensity-based Cost Functions. *Handbook of Medical Imaging: Processing and Analysis*. New York: Academic. 529-536; 2000.



- [74] Legg, P. A., Rosin, P. L., Marshall, D. and Morgan, J. E. Incorporating neighbourhood feature derivatives with mutual information to improve accuracy of multi-modal image registration. *Medical Imaging Understanding and Analysis*. 2008. 39-43.
- [75] Sandoval, Z. L. and Dillenseger, J. L. Evaluation of Computed Tomography to Ultrasound 2D Image Registration for Atrial Fibrillation Treatment. *Computing in Cardiology Conference (CinC)*. 2013. 245-248.
- [76] Russakoff, D. B., Rohlfing, T., Adler, J. R. and Maurer, C. R. Intensity-based 2D-3D Spine Image Registration Incorporating a Single Fiducial Marker. *Academic radiology*. 12(1): 37-50.
- [77] Li, F., Lang, P., Rajchl, M., Chen, E. C., Guiraudon, G. and Peters, T. M. Towards Real-time 3D US-CT Registration on the Beating Heart for Guidance of Minimally Invasive Cardiac Interventions. *International Society for Optics and Photonics. SPIE Medical Imaging*. 2012.
- [78] Li, F., Rajchl, M., White, J. A., Goela, A. and Peters, T. M. Generation of Synthetic 4D Cardiac CT Images for Guidance of Minimally Invasive Beating Heart Interventions. In *Information Processing in Computer-Assisted Interventions*. Heidelberg: Springer-Berlin. 11-20; 2013.
- [79] Ourselin, S., Roche, A., Prima, S. and Ayache, N. Block Matching: A General Framework to Improve Robustness of Rigid Registration of Medical Images. In: Delp, S., DiGoia, A. and Jaramaz, B. ed. *Medical Image Computing and Computer-Assisted Intervention-MICCAI 2000*. Heidelberg: Springer-Berlin. 557-566; 2000.
- [80] Woods, R. P., Grafton, S. T., Watson, J. D., Sicotte, N. L. and Mazziotta, J. C. Automated Image Registration: II. Intersubject Validation of Linear and Nonlinear Models. *Journal of Computer Assisted Tomography*. 1998. 22(1): 153-165.
- [81] Sotiras, A., Davatzikos, C. and Paragios, N. Deformable Medical Image Registration: A Survey. *IEEE Transactions on Medical Imaging*. 2013. 32(7): 1153-1190.
- [82] Crum, W. R., Hartkens, T. and Hill, D. L. G. Non-rigid image registration: theory and practice. *The British Journal of Radiology*. 2004. 77(2): 140-53.

- [83] Bro-Nielsen, M. *Medical Image Registration and Surgery Simulation*. PhD Thesis, Department of Mathematical Modelling, Technical University of Denmark; 1997.
- [84] Powell, M. J. D. An Iterative Method of Finding Stationary Values of a Function of Several Variables. *The Computer Journal*. 1962. 5(2): 147–151.
- [85] Meyer, C. R., Leichtman, G. S., Brunberg, J. A., Wahl, R. L. and Quint, L. E. Simultaneous Usage of Homologous Points, Lines, and Planes for Optimal, 3-D, Linear Registration of Multimodality Imaging Data”. *IEEE Transactions on medical imaging*. 1995. 14(1): 1-11.
- [86] Slomka, P., Hurwitz, G., Stephenson, J. and Craddock, T. Automated Alignment and Sizing of Myocardial Stress and Rest Scans to Three-dimensional Normal Templates using an Image Registration Algorithm. *The Journal of nuclear medicine*. 1995. 36(6): 115-1122.
- [87] Hoh, C. K., Dahlbom, M., Harris, G., Choi, Y., Hawkins, R. A., Phelps, M. E. and Maddahi, J. Automated Iterative Three-dimensional Registration of Positron Emission Tomography Images. *Journal of nuclear medicine*. 1993. 34(11): 2009-2018.
- [88] P. Viola. *Alignment by Maximisation of Mutual Information*. PhD thesis. Artificial Intelligence Laboratory, Massachusetts Institute of technology; 1995.
- [89] Maes, F., Collignon, A., Vandermeulen, D., Marchal, G. and Suetens, P. Multimodality image registration by maximization of mutual information. *IEEE Transactions on Medical Imaging*. 1997. 16(2): 187-198.
- [90] Maes, F., Vandermeulen, D. and Suetens, P. Comparative Evaluation of Multiresolution Optimization Strategies for Multimodality Image Registration by Maximization of Mutual Information. *Medical image analysis*. 1999. 3(4): 373-386.
- [91] Klein, S., Staring, M. and Pluim, J. P. W. Evaluation of Optimization Methods for Nonrigid Medical Image Registration using Mutual Information and B-splines. *IEEE Transactions on Image Processing*. 2007. 16(12): 2879-2890.
- [92] Pluim, J. P. W., Maintz, J. A. and Viergever, M. A. Mutual Information Matching in Multiresolution Contexts. *Image and Vision Computing*. 2001. 19(1): 45-52.

- [93] Thevenaz, P. and Unser, M. Optimization of Mutual Information for Multiresolution Image Registration. *IEEE Trans. Imag. Process.* 2000. 9(12): 2083-2099.
- [94] Wachowiak, M. P., Smolíková, R., Zheng, Y., Zurada, J. M. and Elmaghraby, A. S. An Approach to Multimodal Biomedical Image Registration Utilizing Particle Swarm Optimization. *IEEE Transactions on Evolutionary Computation.* 2004. 8(3): 289-301.
- [95] Anna, W., Tingjun, W., Jinjin, Z. and Silin, X. A Novel Method of Medical Image Registration Based on DTCWT and NPSO. *Fifth International Conference on Natural Computation (ICNC'09).* 2009. 5: 23-27.
- [96] Ayatollahi, F. , Shokouhi, S. and Ayatollahi, A. A New Hybrid Particle Swarm Optimization for Multimodal Brain Image Registration. *Journal of Biomedical Science and Engineering.* 2012. 5(4): 153-161.
- [97] Goshtasby, A. A., and Nikolov, S. Guest editorial: Image fusion: Advances in the state of the art. *Information. Fusion,* 2007. 8(2): 114-118.
- [98] Bhavana, V., and Krishnappa, H. K. Multi-Modality Medical Image Fusion – A Survey. *International Journal of Engineering Research & Technology.* 2015.4(2): 778-781.
- [99] Swathi, P. S., Sheethal, M. S., and Vince, P. Survey on Multimodal Medical Image Fusion Techniques. *International Journal of Computer Science Engineering and Technology.* 2016. 6(1): 33-39
- [100] El-Gamal, F. El-Z. A., Elmogy, M., and Atwan, A. Current trends in medical image registration and fusion. *Egyptian Informatics Journal,* 2016. 17(1): 99-124.
- [101] Hiremath, P. S., Akkasaligar, P. T. and Badiger, S. Speckle Noise Reduction in Medical Ultrasound Images. In: Gunarathne, G. ed. *Advancements and Breakthroughs in Ultrasound Imaging.* 201-241; 2011.
- [102] Lee, J. S. Refined filtering of image noise using local statistics. *Computer Vision, Graphics and Image Processing.* 1981. 15(4): 380-389.
- [103] Perona, P. and Malik, J. Scale Space and Edge Detection using Anisotropic Diffusion. *IEEE Trans. Pattern Anal. Machine Intell.* 1990. 12(7): 629-639.
- [104] Yu, Y. and Acton, S. T. Speckle Reducing Anisotropic Diffusion. *Image Processing, IEEE Transactions on.* 2002. 11(11): 1260-1270.

- [105] Zuiderveld, K. Contrast Limited Adaptive Histogram Equalization. *In Graphics gems IV .Academic Press Professional, Inc.* 474-485.
- [106] Kaur, M. and Kaur, J. Survey of Contrast Enhancement Techniques based on Histogram Equalization. *International Journal of Advanced Computer Science and Application.* 2011. 2( 7): 137-141.
- [107] Min, B. S., Lim, D. K., Kim, S. J. and Lee, J. H. A Novel Method of Determining Parameters of CLAHE based on Image Entropy. *International Journal of Software Engineering and Its Applications.* 2013. 7(5): 113-120.
- [108] Serra, J. *Image Analysis and Mathematical Morphology.* Academic Press, Inc. 1983.
- [109] Ming, C. T., Omar, Z. and Kadiman, S. Efficient Morphological- Based Edge Detection Algorithm For Computed Tomography Cardiac Images. *IEEE International Conference on Signal and Image Processing Applications (ICSIPA).* 19-21 Oct. 2015. 423-428.
- [110] Kumar, M. and Sukhwinder, S. Edge Detection And Denoising Medical Image Using Morphology. *International Journal of Engineering Sciences & Emerging Technologies.* 2012. 2(2): 66-72.
- [111] Palani, D., Venkatalakshmi, K. and Venkatraman, E. Implementation and Comparison of Different Segmentation Algorithms for Medical Imaging. *International Conference on Innovations in Engineering and Technology.* 21-22 March. 2014. 1217-1223.
- [112] Xu, C. and Prince, J. L. Gradient vector flow: A New External Force for Snakes. *Conference on Computer Vision and Pattern Recognition.* IEEE Proceedings Computer Society. 1997. 66-71.
- [113] Xu, C. and Prince, J. L. Snakes, Shapes, and Gradient Vector Flow. *IEEE Transactions on Image Processing.* 1999. 7(3): 359-369.
- [114] Kass, M., Witkin, A. and Terzopoulos, D. Snakes: Active contour models. *Int. J. Comput. Vis.* 1987. 1(4): 321-331.
- [115] Cohen, I., Cohen, L. D. and Ayache, N. Using Deformable Surfaces to Segment 3-D Images and Infer Differential Structures. *Computer Vision- ECCV'92.* Heidelberg: Springer- Berlin. 1992. 648-652.
- [116] Davatzikos, C. and Prince, J. L. An Active Contour Model for Mapping the Cortex. *IEEE Trans.on Med. Imag.* 1995. 14(1): 65-80.

- [117] Abrantes, A. J. and Marques, J. S. A Class of Constrained Clustering Algorithms for Object Boundary Extraction. *Image Processing, IEEE Transactions on*. 1996. 5(11): 1507-1521.
- [118] Courant, R. and Hilbert, D. *Methods of Mathematical Physics*. volume 1. New York: Interscience. 1953.
- [119] Lowe, D. G. Distinctive Image Features from Scale-invariant Keypoints. *International journal of computer vision*. 2004. 60(2): 91-110.
- [120] Hartley, R. and Zisserman, A. *Multiple view geometry in computer vision*. Cambridge university press. 2003.
- [121] Fischler, M. A. and Bolles, R.C. Random Sample Consensus: A Paradigm for Model Fitting with Applications to Image Analysis and Automated Cartography. *Communications of Association of Computing Machines*. 1981. 24(6): 381-395.
- [122] Bradski, G. and Kaehler, A. *Learning OpenCV*. Sebastopol: O'Reilly Media Inc. 2008; 194-221.
- [123] Ming, C. T., Omar, Z. and Kadiman, S. SIFT and homographic transform-based cardiac image registration. *2014 IEEE Conference on Biomedical Engineering and Sciences (IECBES)*. 8-10 December, 2014. 970-974.
- [124] Collignon, A., Maes, F., Delaere, D., Vandermeulen, D., Suetens, P. and Marchal, G. Automated Multimodality Medical Image Registration using Information Theory. *14th Int. Conf. Information Processing in Medical Imaging (IPMI'95)*. Ile de Berder, France: Computational Imaging and Vision (vol. 3). June 1995. 263-274.
- [125] Maes, F., Collignon, A., Vandermeulen, D., Marchal, G. and Suetens, P. Multimodality Image Registration by Maximization of Mutual Information *IEEE Trans. Med. Imag.* 1997. 16(2): 187-198.
- [126] Viola, P. and Wells III, W. M. Alignment by Maximization of Mutual Information. *Proc. 5th Int. Conf. Computer Vision*. June 1995. Cambridge, MA. 16-23.
- [127] Wells, W. M., Viola, P., Atsumi, H., Nakajima, S. and Kikinis, R. Multimodal Volume Registration by Maximization of Mutual Information. *Medical Image Analysis*. 1996. 1(1): 35-51.

- [128] Maes, F., Vandermeulen, D. and Suetens, P. Medical Image Registration using Mutual Information. *Proceedings of the IEEE*. 2003. 91(10): 1699-1722.
- [129] Studholme, C., Hill, D. L. and Hawkes, D. J. An Overlap Invariant Entropy Measure of 3D Medical Image Alignment. *Pattern recognition*. 1999. 32(1): 71-86.
- [130] Hill, D. L., Hawkes, D. J., Harrison, N. A. and Ruff, C. F. A Strategy for Automated Multimodality Image Registration Incorporating Anatomical Knowledge and Image Characteristics. In: Barrett, H. H. and Gmitro, A. F. Eds. *Information Processing in Medical Imaging (vol. 687)*. Berlin: Springer-Verlag. pp. 182–196; 1993.
- [131] Kosiński, W., Michalak, P. and Gut, P. Robust Image Registration based on Mutual Information Measure. *Journal of Signal and Information Processing*. 2012. 3(02): 175.
- [132] Matsuura, N., Horiguchi, J., Yamamoto, H., Hirai, N., Tonda, T., Kohno, N. and Ito, K. Optimal Cardiac Phase for Coronary Artery Calcium Scoring on Single-source 64-MDCT Scanner: Least Interscan Variability and Least Motion Artifacts. *American Journal of Roentgenology*. 2008. 190(6): 1561-1568.
- [133] Francone, M., Napoli, A., Carbone, I., Cavacece, M., Nardis, P.G., Lanciotti, K., Visconti, S., Bertolotti, L., Di Castro, E., Catalano, C. and Passariello, R. Noninvasive Imaging of the Coronary Arteries using a 64-row Multidetector CT Scanner: Initial Clinical Experience and Radiation Dose Concerns. *Radiology Medicine*. 2007. 112(1):31–46.
- [134] Retrieved from: <http://www.healthcare.siemens.com/services/it-standards/dicom-conformance-statements-multi-modality-workplaces>
- [135] Retrieved from: <http://www.siaronmedical.com/product/syngo-multimodality-workplace-2007-sm-0017>
- [136] Retrieved from: <https://www.mathworks.com/help/images/ref/imregister.html>
- [137] Viera, A. J. and Garrett, J. M. Understanding interobserver agreement: the kappa statistic. *Fam Med*. 2005. 37(5): 360-363.
- [138] Choi, S. and Kim, C. Automatic Initialization Active Contour Model for the Segmentation of the Chest Wall on Chest CT. *Healthcare Informatics Research*. 2010. 16(1): 36-45.

- [139] Athertya, J. S and Kumar, G. S. Automatic Initialization for Segmentation of Medical Images based on Active Contour. *2014 IEEE Conference on Biomedical Engineering and Sciences (IECBES)*.8-10 December, 2014. 446-451.
- [140] Li, B. and Acton, S.T. Active Contour External Force using Vector Field Convolution for Image Segmentation. *IEEE Transactions on Image Processing*. 2007. 16(8): 2096-2106.
- [141] Han, X., Xu, C. and Prince, J. L. Fast Numerical Scheme for Gradient Vector Flow Computation using a Multigrid Method. *IEEE Trans on Image Processing*. 2007. 1(1): 48-55
- [142] Ren, D., Zuo, W., Zhao, X., Lin, Z. and Zhang, D. Fast Gradient Vector Flow Computation based on Augmented Lagrangian Method. *Pattern Recognition Letters*. 2013. 34(2):219-225.
- [143] Bay, H., Tuytelaars, T., Gool, L.V. (2006). SURF: Speeded up robust features. *In Computer Vision –ECCV 2006 : 9th European Conference on Computer Vision*. 7-13 May 2006. Springer, Part II, 404-417.
- [144] Morel, J. M., and Yu, G. ASIFT: A new framework for fully affine invariant image comparison. *Journal on Imaging Sciences*. 2009: 2 (2): 438-469.
- [145] Guoshen, Y., and Jean-Michel, M. ASIFT: An Algorithm for Fully Affine Invariant Comparison, *Image Processing On Line*. 2011.1: 11-38.